MIDMARK®

Installation Instructions

9A272002 BASE RAIL ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A272002	Base Rail Assembly	1 pair
• 040-0250-133	1/4"-20 x1/2" hex flange head bolt (Grade 5)	6
003-1028-00	I / O Instructions	1

REQUIRED TOOLS

3/8" Socket or Wrench
Punch
Hammer
Pliers

INTRODUCTION

To provide a secure, stationary support for mounting certain accessories such as I.V. Pole, Vision Block Screen, Instrument Tray, and Welch Allyn Bracket.

WARNING

Do not install on same side of table that has a 9A25400X Seat Rail. Remove any Seat Rails before installing the Base Rail. Multiple attachment of accessories on a single rail is not recommended. Failure to comply may result in personal injury or equipment damage.

INSTALLATION

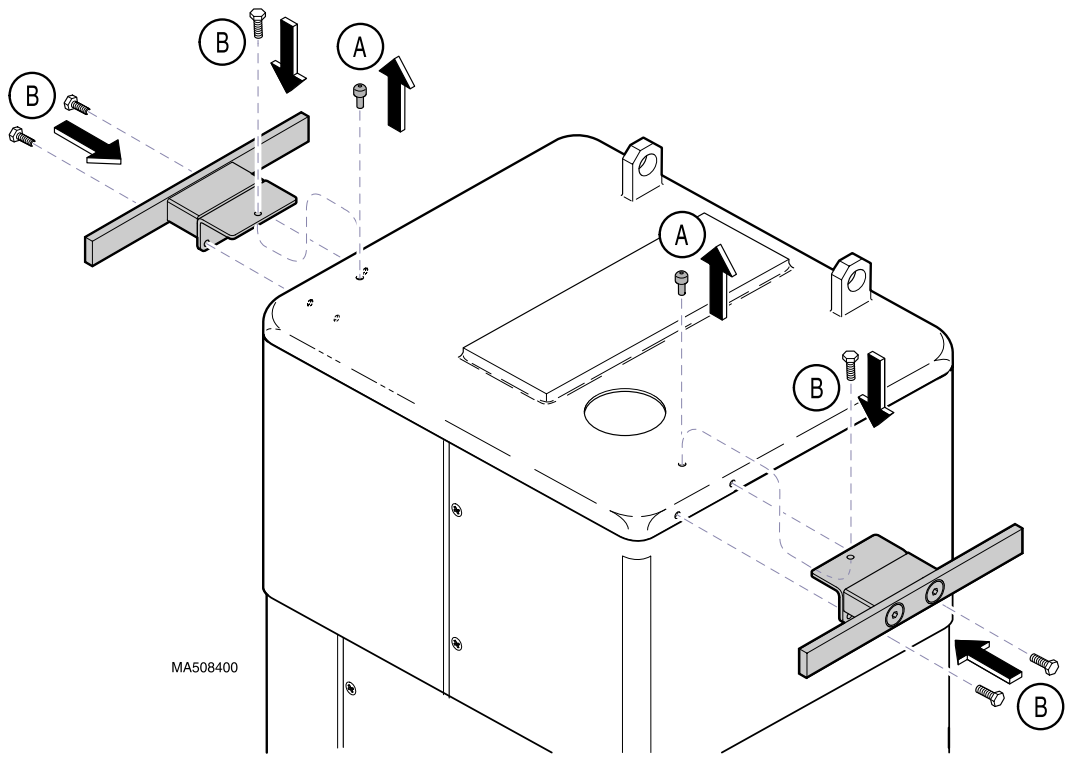

NOTE

For ease of installation, move TABLE, BACK, TILT and FOOT functions fully UP.

A. Using punch and pliers, remove black plastic rivets from mounting holes by taping them inward.

NOTE

Base rails are inter-changeable, either can be used on the patient's right or left side.

B. Place base rail in position and install mounting screws.

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 1999